

Content

1.	Identification.....	25
2.	General notes.....	25
3.	Notes.....	27
3.1	Safety instructions.....	27
3.2	Instructions for the safe use of the product.....	27
4.	Scope of delivery and product overview.....	28
4.1	Scope of delivery.....	28
4.2	Marking/Label.....	28
4.3	Product overview.....	29
5.	Operation.....	30
5.1	Insert seat board.....	30
5.2	Grip and support positions when walking and standing inside the rollator.....	30
5.3	Grip and support positions when walking and standing outside the rollator.....	31
5.4	Standing up and sitting down.....	31
5.5	Brake system.....	32
5.5.1	Braking and locking the brake with the brake handles.....	32
5.5.2	Braking and locking the brake with the brake bar.....	33
5.5.3	Disassembling/assembling the brake bar.....	33
5.5.4	Adjusting and checking the brake system.....	34
5.6	Locking the direction.....	35
5.7	Tripping with the rollator.....	35
6.	Maintenance and reuse.....	36
6.1	Maintenance.....	36
6.2	Maintenance schedule.....	36
6.2.1	Daily visual inspection.....	36
6.2.2	Function tests.....	36
6.2.3	Cleaning.....	36
6.2.4	Disinfection.....	38
6.3	Reuse.....	38
7.	Storage and shipping.....	38
8.	Disposal.....	38
9.	Technical data and list of materials.....	39
9.1	Technical data.....	39
9.2	Materials used.....	39
10.	Warranty and guarantee.....	40
10.1	Warranty.....	40
10.2	Guarantee.....	40
11.	Note on the obligation to report incidents.....	41
12.	Accessories.....	42
13.	Test protocol for reuse.....	44

1. Identification

Manufacturer: Saljol GmbH
Product: Indoor Rollator
Type: Indoor rollator, walking frame, serving trolley and commode chair
Article name: Indoor Rollator
Version: 2025

Manufacturer: Saljol GmbH
Frauenstraße 32
D-82216 Maisach
Phone: +49 (0)8141 317740
Fax: +49 (0)8141 3177411
Mail: hallo@saljol.de
Web: www.saljol.de

Swiss representative and importeur:

 CON GmbH
Talgut-Zentrum 7
CH-3063 Ittigen

Formalities of the operating instructions

Version/Revision: 2025.02
Creation date: 07.08.2025

Information is correct at the time of going to press.

We reserve the right to make technical changes. Technical drawings and photos may differ from reality.

©2025 Saljol GmbH: all rights reserved. Reprinting, including excerpts, only with the permission of Saljol GmbH

2. General Notes

Purpose

The Indoor Rollator by Saljol has been developed for indoor use and is only suitable for use on firm ground. With the help of the Indoor Rollator by Saljol, people can stand and walk again and the user can rest on the integrated seat and move around in a seated position. Everyday routine tasks can be performed by users with the Saljol Indoor Rollator without having to rely on assistance from others.

Applications: The Indoor Rollator by Saljol is designed to cover a wide range of health problems. It is specially designed for people who need extra stability support when walking.

Indication

The Indoor Rollator by Saljol is designed exclusively for use as a walking aid and is particularly suitable for patients with limited mobility due to physical impairments, limitations of the active or passive musculoskeletal system and diseases such as arthritis, osteoporosis, muscle weakness, stroke or Parkinson's disease.

Contraindication

The Saljol Indoor Rollator is not suitable for people with very weak arm strength, significant cognitive impairment, or very poor balance. The use and application of the Saljol Indoor Rollator should be assessed and instructed by a doctor or therapist.

Service life

With proper use, regular care and maintenance by a specialist company and compliance with the safety instructions, the expected lifespan of the Indoor Rollator is up to 4 years. If the rollator is still in proper condition after 4 years, you can continue to use it.

Responsibility

As the manufacturer, we can only consider ourselves responsible for the safety, reliability and usability of the rollator if changes, expansions, repairs and maintenance work are carried out regularly and only by authorized specialists and if the rollator is used properly in compliance with all instructions for use.

Declaration of conformity



Saljol, as the manufacturer of the product, declares that the Indoor Rollator fully complies with the requirements of Medical Device Regulation (2017/745) (status 2022). A CE Declaration of Conformity can be found on our homepage www.saljol.de.

The manufacturer/responsible person declares that the following products are approved with Product designation Indoor Rollator, Version 2025

Saljol Indoor Rollator WR43	Velvet Grey	4058789015834
Saljol Indoor Rollator WR50	Velvet Grey	4058789015803
Saljol Indoor Rollator WR53	Velvet Grey	4058789015810
Saljol Indoor Rollator WR56	Velvet Grey	4058789015827
Saljol Indoor Rollator WR43	Champagne Gold	4058789015872
Saljol Indoor Rollator WR50	Champagne Gold	4058789015841
Saljol Indoor Rollator WR53	Champagne Gold	4058789015858
Saljol Indoor Rollator WR56	Champagne Gold	4058789015865

comply with the following harmonised standards: EN ISO 11199-2:2021. Walking aids manipulated by both arms – Requirements and test methods – Part 2: Rollators; Seat and handles meets the biological assessment according to ISO 10993-5: 2009-10

3. Notes

3.1 Safety instructions

The instruction manual contains safety notes that are marked twice: by a symbol and by a signal word. The symbol informs you about the type of notice. The signal word explains more details, for example the severity of an impending risk.



Caution/Important

Possibly dangerous situation (minor injuries or material damage), commitment to a particular behaviour or activity for the safe use of the rollator



Note

Application tips and useful information

3.2 Instructions for the safe use of the product

For safe use of the product, please keep the following in mind:



Restrictions on use

- The maximum user weight must not exceed 150 kg for WR50, WR53 and WR56 and 120 kg for WR43.
- The rollator is designed only for indoor use.
- Never use in the presence of flammable/combustible and burning substances.



Accident prevention

- Only use the rollator for the defined purpose.
- Only use the rollator if it is in perfect technical condition.
- It is prohibited to make any constructive changes to the rollator, unless you have the written consent of the manufacturer Saljol.
- While adjusting the rollator, be careful not to pinch your fingers or other body parts on the moving parts.
- Make sure that the parking brake is activated when you sit down on the rollator.
- Make sure that there is no direct skin contact with the seat surface when using this product. The thighs and bottom should always be covered with clothing to avoid skin squeezing.
- Make sure that the seat board does not restrict legroom when walking. The seat board should be placed upright in the rollator.
- All four wheels must be in contact with the ground at all times. Only in this way the rollator is safely balanced which prevents accidents.
- Always apply the parking brake when you stop or park the rollator.

4. Scope of delivery and product overview

4.1 Scope of delivery


The equipment of our products may vary depending on the country and configuration to meet local requirements. Therefore, the scope of delivery may differ.

1x Saljol Indoor Rollator	1x Cork handrail padding (pre-assembled)*
1x Seat board with felt pad	1x Brake bar (pre-assembled)
1x Tray with felt pad*	1x instruction manual
1x Small bag (pre-assembled)*	

*Not included in the scope of delivery, depending on the variant

4.2 Marking/Label

The serial number and EAN code are on a label on the inside of the frame. The label also contains important information about the product: manufacturer's details about Saljol, production date, maximum user weight, product size and seat height. The label must not be removed.

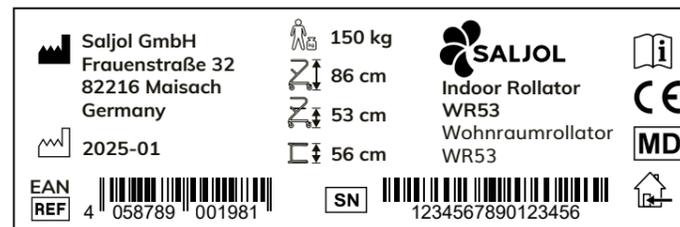

The following symbols can be found, partly in combination with further information, on the marking of the Indoor Rollator and on the packaging to identify important properties.

Manufacturer of the product	Product width
Production date	Serial number
Order number/item number	Observe instruction manual
Maximum user weight	CE marking
Product height	Medical device
Seat height	Product only suitable for indoors

4.3 Product overview



*Not included in the scope of delivery, depending on the variant

Figure: Saljol Indoor Rollator

5. Operation

Inventory

Take the Saljol Indoor Rollator out of the box and check if anything is missing. Compare with the scope of delivery, described under 4.1 on page 28. If any part is missing or damaged, contact your dealer or Saljol immediately.

5.1 Insert seat board



Important

- Check that the seat board is firmly in place before you sit down.
- Never lean on the area of the seat board marked in the picture, otherwise it may fold downwards.



5.2 Grip and support positions when walking and standing inside the rollator



5.3 Grip and support positions when walking and standing outside the rollator



5.4 Standing up and sitting down



Important

When standing up and sitting down, the parking brake must be activated.



5.5 Brake system



Important

When you sit on the Indoor Rollator to rest, it is absolutely necessary to lock the brakes.

As the brake handles and the brake bar are one braking system, the brake bar also moves when the brake handles are used. If you use the brake bar, both brake handles move.

5.5.1 Braking and locking the brake with the brake handles



Braking

To brake the rollator, simply pull both brake handles upwards towards the frame.



Lock the brake

To apply the parking brake, press both brake handles down until you overcome a slight resistance. Both rear wheels are now locked.



Release the brake

To release the parking brake, pull both brake handles upwards.

5.5.2 Braking and locking the brake with the brake bar



Braking

To brake the rollator, simply pull the brake bar upwards towards the frame at any point. The brake bar brakes both rear wheels simultaneously.



Lock the brake

To apply the parking brake, pull the brake bar upwards until you overcome a slight resistance. Both rear wheels are now locked.



Release the brake

To release the parking brake, press the brake bar down.

5.5.3 Disassembling/assembling the brake bar

Disassembly



Turn the rollator over and place it on the handrail. Now unscrew the screws on both handles with an allen key size 3 mm.



Now you can remove the brake bar.

Keep the brake bar together with the screws in case you want to reinstall the brake.

Assembly

To refit the brake bar, insert the brake bar into the holes provided (picture above) and tighten both screws on the brake handles.

5.5.4 Adjusting and checking the brake system

Turn the rollator over and place it on the handrail. Have a allen key size 4 mm, a 10 mm open-end spanner and a ratchet with a 10 mm socket ready.



First remove the brake bar as described in point 5.5.3, if it is mounted.

1. loosen the screw of the desired brake handle with the screwdriver and pull out the brake housing.
2. loosen the lock nut with the open-end spanner
3. unscrew the tension end sleeve with the ratchet with a 10 mm nut (brake becomes tighter) or screw it in (brake becomes smoother)
4. check brake force
5. repeat point 3-4 until the desired setting is found
6. tighten the lock nut
7. insert the brake housing and tighten the screw
8. mount the brake bar again, if desired



Caution

The brake is correctly adjusted if the rear wheels lock when the brake is applied and do not turn when pushed.



Information

Here you can find a video explaining the brake adjustment: <https://youtu.be/i9L5vHUD15s> or scan the QR code.



5.6 Locking the direction



To lock the direction of the rear wheels, press down the pedal levers on both sides until you hear a soft „click“ sound. As soon as you drive straight ahead, the wheels lock automatically.



To release the directional lock, press the central locking lever.

5.7 Tripping with the rollator



It is permitted to move around your home while sitting on the Saljol Indoor Rollator. This is how you move safely through your home:

1. check that the seat board is firmly fixed
2. lock the brakes
3. sit down
4. release the brakes

Now you can move around the rooms with your feet

6. Maintenance and reuse

6.1 Maintenance

Although the Saljol Indoor Rollator is generally robust and durable due to corrosionprotected materials, it still requires regular cleaning and maintenance. To ensure that your rollator can be operated safely at all times, we recommend that you regularly carry out the checks specified in the maintenance schedule. Insufficient or neglected care and maintenance of the rollator can lead to an impairment of safety and limit liability. Please note, however, that the maintenance plan does not contain precise information on the actual amount of work required on the rollator. It is therefore advisable to consider any problems or additional maintenance needs you notice on the rollator accordingly and seek professional help if necessary. By carrying out the recommended maintenance regularly and paying attention to any deviations, you can ensure that your rollator is always in optimal condition and provides you with safe support. Saljol reserves the right to limit guarantee claims if the rollator has not been regularly maintained.

6.2 Maintenance schedule

6.2.1 Daily visual inspection

The daily visual inspection of the rollator should be carried out before each use. It helps to check main components (frame, brakes, handles, seat and wheels) for any damage, signs of wear or other problems before they become major problems. Look for changes or missing elements and if in doubt ask your dealer, Saljol distributor or Saljol GmbH.

6.2.2 Function tests

Function tests help to ensure that all functions of the rollator are working properly. If the tested component does not function properly, it must be repaired immediately by yourself or by qualified personnel. We recommend that the Indoor Rollator is subjected to function tests at least once a month, ideally twice. The function tests include:

- Brake test: check the rollator's brakes to make sure they are working properly. Make sure that the rollator can be brought to a stop quickly and safely on both sides if necessary. The parking brake should lock both rear wheels and prevent the rollator from rolling away.
- Tyre test: Check the rollator's tyres to ensure that they turn easily and show no signs of heavy wear or damage. Defective tyres should be replaced immediately.

6.2.3 Cleaning

Depending on the degree of soiling, but at least monthly, the entire rollator must be cleaned. Cleaning of heavier dirt can be done with warm water and a sponge. In case of stubborn dirt, a commercial cleaning agent can be added to the water. Disinfectants can be used without any problems. Plastic parts are best cleaned with a commercially available plastic cleaner. Please follow the instructions for use of the cleaning agent used.

Frame

Cleaning can be done with the supplied care cloth, or for heavier dirt, with warm water and a sponge. In case of stubborn soiling, a commercial cleaning agent can be added to the water. Disinfectants can be used without any problems. Plastic parts are best cleaned with a commercially available plastic cleaner. Please follow the instructions for use of the cleaning agent used.



Important

Never use aggressive cleaning agents such as solvents/abrasives or hard brushes.

Wheels

Clean the wheels with warm water and a mild solvent. If necessary, use a plastic brush, never a wire brush.



Important

Never clean the rollator with a high-pressure/steam cleaner!

Cork TPE

Dust and other particles can settle on the surface of cork TPE products during storage and cause a „grey haze“. This is not a product defect but can be easily removed. Proper care and cleaning of cork TPE coated elements will help extend the life of the material. Loose dirt can be removed with a soft, dry cloth or a soft brush; heavier dirt with a soft cloth and soap solution. Wring out the cloth well. Avoid rubbing heavily or using abrasive cleaners or sponges as these may damage the cork TPE. To preserve the life of the cork TPE, we recommend regular cleaning and protection from direct sunlight, heat sources and moisture. Cork is a natural material and can also change colour over time under the influence of light and humidity.

Tray/Seat board with felt pad

Loose soiling can be removed with a soft, dry cloth or a soft brush; heavier soiling can be removed with a soft cloth and soap solution. Wring out the cloth well. Avoid rubbing hard or using abrasive cleaning agents or sponges.

6.2.4 Disinfection

The Indoor Rollator can be disinfected with standard household disinfectants. The Robert Koch list of approved disinfectants can be found at <http://www.rki.de>. Allow the rollator to air dry and observe the exposure time of the disinfectant you are using.

6.3 Reuse

The Saljol Indoor Rollator is suitable for reuse. The number of times the rollator can be used again depends on the state of wear of the material and the functional capability of the product. Before using the rollator again, make sure that it has been cleaned and disinfected. All visible dirt should be removed and the rollator should then be treated with a suitable disinfectant to ensure that it is free of germs and bacteria. It is also important that you carry out all the checks listed in point 6.2 „Maintenance schedule“ to ensure that the rollator is in perfect condition. The Saljol Indoor Rollator is resistant to the agents used for reuse.

7. Storage and shipping

When not in use, keep the rollator upright, in a dry place, out of reach of children or third parties. If the Indoor Rollator needs to be stored or shipped, it is advisable to keep the original packaging and store it for these purposes so that it is available when needed. Then your rollator is optimally protected against environmental influences during storage or transport.

8. Disposal

Dispose materials separately by type in the designated collection systems. Please dispose hazardous waste in the designated collection systems.

9. Technical data and list of materials

9.1 Technical data

Indoor Rollator	WR43	WR50	WR53	WR56
Handle height	78 cm	80 cm	86 cm	92 cm
Seat height	43 cm	50 cm	53 cm	56 cm
Recommended for body height	135–155 cm	145–165 cm	150–180 cm	170–200 cm
Max. user weight	120 kg	150 kg	150 kg	150 kg
Length	61 cm	61 cm	61 cm	61 cm
Width bottom	56 cm	56 cm	56 cm	56 cm
Width top	51 cm	51 cm	51 cm	51 cm
Distance between the handles	43 cm	43 cm	43 cm	43 cm
Weight without accessories	9.4 kg	9.6 kg	9.8 kg	10.0 kg
Maximum load of the bag	0.5 kg	0.5 kg	0.5 kg	0.5 kg
Wheels (diameter x width)	12.5 x 3 cm, grey, anti-slip TPE-wheels			
Turning circle	69 cm	69 cm	69 cm	69 cm

9.2 Materials used

Frame	Steel Q235
Brake bar	Aluminum 6061-T6
Brake handle	Thermoplastic elastomers (TPE) with 20–30% cork
Brake	Plastic – polyamide
Seat board	Birch
Tray	Birch
Felt pads	90% wool +10 % Polyester
Bag	Polyester + cork
Cork handrail pad	100% Polyester + cork
Rims	Plastic – polyamide
Wheels	Thermoplastic polyurethane (TPU)

10. Warranty and guarantee

10.1 Warranty

If the purchased item is defective, the provisions of the statutory liability for defects shall apply. Insofar as you have purchased the goods from a specialist retailer, please contact your seller immediately; if you have purchased directly from Saljol, please contact Saljol directly, Tel. +49 (0)8141 317740. Visible defects must be reported in writing within ten days of delivery, hidden defects within ten days of their discovery. The above-mentioned deadlines are preclusive deadlines. Saljol shall be entitled to decide whether a defect, if any, shall be remedied by rectification or subsequent delivery („subsequent performance“). In all other respects, the provisions in the General Terms and Conditions of Saljol, available at <https://www.saljol.de/en/data-protection/>, shall apply.

10.2 Guarantee

In addition to the statutory guarantee claims and without limiting them, Saljol gives a guarantee of 2 years from the date of purchase on this product. You also have the option to extend this guarantee by a further 2 years if you register the rollator online no later than 14 days after the date of purchase. You can register at www.saljol.de/en/extended-warranty/

Scope of the guarantee

We guarantee that the product will be free from defects in material, workmanship and function within the guarantee period. If a defect occurs during the guarantee period, we will, at our own discretion, either repair the product free of charge or, if necessary, replace it with a new one. Excluded from the guarantee are parts subject to wear and tear such as brake mechanism and tyres.

These guarantee conditions only apply to products purchased in Germany, provided they were purchased from Saljol directly or from an authorised specialist dealer.

The seller will provide information on the guarantee conditions for products purchased abroad. Guarantee services and replacement deliveries for guarantee reasons do not result in an extension of the guarantee period.

Exclusion of the guarantee

The right to claim under guarantee expires if the rollator has been improperly maintained or repaired by an untrained person or if the product has been operated with non-original accessories. Incorrect set-up or installation due to non-observance of the operating instructions, use contrary to the intended purpose or improper use or care of the product will result in a loss of guarantee, as will external influences (e.g. transport damage, damage due to impacts and blows, weather influences).

11. Note on the obligation to report incidents

Please note that all serious incidents occurring in connection with the product must be reported to the manufacturer and the competent authority. Serious incidents in the sense of the law are all adverse events that have one of the following consequences: Death, life-threatening injury, permanent bodily damage and chronic illness.

In the Federal Republic of Germany, please inform:

- your local distributor, Saljol sales partner or
Saljol GmbH, Frauenstr. 32, D-82216 Maisach; www.saljol.de
- the Federal Institute for Drugs and Medical Devices (BfArM),
Kurt-Georg-Kiesinger-Allee 3, 53175 Bonn; www.bfarm.de

In EU Member States, please inform:

- your local distributor, SALJOL sales partner or
Saljol GmbH, Frauenstr. 32, D-82216 Maisach; www.saljol.de
- the authority responsible for incidents involving medical devices in your country

12. Accessories



Note

The following accessories are available for the Indoor Rollator in sizes WR43, WR50, WR53 and WR56.



Tray with felt pad

The sturdy wooden tray can hold up to 20 kg and has a large usable surface. The tray turns the indoor rollator into a serving trolley with which you can even drive over the table and place the tray safely – without the risk of crushing your fingers.



Designer bags from Jost

Turn your indoor rollator into an eye-catcher! The designer bags from Jost are available with beige imitation leather or in transparent PVC. Transport items up to 20 kg load weight safely stowed through your home. You can hang the bag both on the handle and directly under the seat.



Back roll

The back roll can be attached to the frame of the Indoor Rollator with a zipper. This makes the rollator a comfortable movable chair. It can also be used as impact protection on the side tubes or the crossbar. Available in woven fabric grey and imitation leather dark brown.



Small bag

Thanks to the detachable, colour-coordinated bag, you always have personal items such as keys, mobile phone or handkerchiefs to hand.



Upholstered seat

With the upholstered seat your Indoor Rollator becomes a comfortable tripping and transfer wheelchair. Ideal for everyone who uses the rollator, e.g. as a kitchen or work chair. The seat has a load capacity of up to 120 kg and is easy to attach and detach. Also available in synthetic leather dark brown. Available in woven fabric grey and imitation leather dark brown.



Cabinet

The cabinet has a load capacity of 20 kg and can simply be hooked into the top of the frame of the Indoor Rollator. With its two storage compartments, the cabinet is ideal for use as a bedside table.



Note

You can order the accessories in our online shop www.saljol.de around the clock or by telephone via our customer service (Mon.-Fri. 9am-4pm) on the number +49 (0)8141 317740 from home. Available accessories may vary depending on the country.

13. Test protocol for reuse

Test protocol for reuse by a qualified specialist.

Question	Yes	No
Does the product have all labels stuck on?		
Do the brakes work?		
Does the directional locking of the wheels work?		
Are the brake handles firm and do not wobble?		
Is the brake bar firm and does not wobble?		

Date

Auditor

Stamp/Signature

